MNA LABORATUVARLARI SAN. TİC, LTD, STİ.

MNA LABORATUVARLARI

TECHNICAL EVALUATION REPORT (65-20-02-R01)

Report No : 65-20-02-R01

Report Date : 17.11.2020

Application No : 65-20-02

1. COMPANY INFORMATION:

LindenCare GmbH

Pempelforter Str. 50, 40211 Düsseldorf Germany

Tel: +0 545 903 26 06

Fax: -

E-mail: a.cansu@kloepfel-consulting.com


2. PPE INFORMATION:

Disposable and non-sterile half mask made of particulate protection filter material.

3. PPE TYPE IDENTIFICATION

EN 149 +A1 Respiratory protective devices - Filtering half masks to protect against particles - Requirements, testing, marking

4. PPE PICTURES

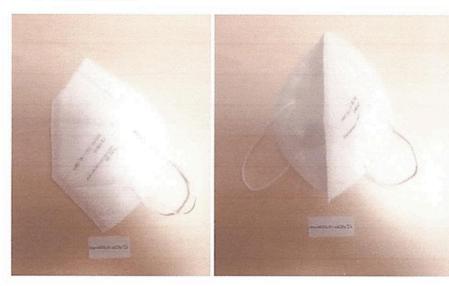

LINDENCARE LP1

5. PPE DIMENSIONS:

LINDENCARE LP1 model has been found to be produced using standard sizes.

6. PPE PRODUCT MATERIAL INFORMATION:

The mask is made of elastic strap, non-woven fabric on the outer and inner layers and filter material on the middle layer.

MNA LABORATUVARLARI



TECHNICAL EVALUATION REPORT (65-20-02-R01)

7. ESSENTIAL HEALTH AND SAFETY REQUIREMENTS

- A visual inspection was made according to EN 149 + A1 for ergonomics.
- Protection levels and degrees are defined by the manufacturer.
- Suitable construction materials were determined by visual inspection according to EN 149 + A1.
- Respiratory protective dimensions are evaluated according to EN 149 + A1.
- Conditioning EN 149 + A1 part 8.3, Penetration EN 149 + A1 part 8.11 (EN 13274-7), Application performance EN 149 + A1 part 8.4, Inward leakage EN 149 + A1 part 8.5, Flammability EN 149 + A1 part 8.6, The carbon dioxide content of the inhaled air EN 149 + A1 part 8.7, Inhalation resistance EN 149 + A1 part 8.9, Exhalation resistance EN 149 + A1 part 8.9 has been tested and evaluated.

8. ANALYSIS AND EVALUATIONS:

EN 149 +A1

TESTS	PARAMETER	PERFORMANCE LEVELS			RESULTS	PERFORMANCE LEVELS	EVALUATION
		FFP1	FFP2	FFP3			
Visual inspection	Shall also the markin supplied by the manu			mation	Appropriate	-	PASS
Total inward	At least 46 out of the 50 individual exercise result	<25	<11	<5	See the table below	FFP2	PASS
leakage	At least 8 out of the 10 individual wearer arithmetic means	<22	<8	<2	See the table below	FFP2	PASS

Total Inward Leakage (%)									
	Exercise 1	Exercise 2	Exercise 3	Exercise 4	Exercise 5	Average			
Subject 1 (As recièved)	0.6	0.0	1.5	1.7	1.8	1.1			
Subject 2 (As recieved)	0.8	0.0	1.5	1.9	1.7	1.2			
Subject 3 (As recieved)	0.9	1.4	1.5	1.1	1.5	1.3			
Subject 4 (As recieved)	0.6	2.1	4.3	1.7	1.7	2.1			
Subject 5 (As recieved)	0.3	3.1	2.1	1.4	1.7	1.7			
Subject 6 (After temperature conditioning)	0.2	0.9	0.7	0.2	1.7	0.7			
Subject 7 (After temperature conditioning)	0.0	1.2	0.6	1.5	0.1	0.7			
Subject 8 (After temperature conditioning)	0.3	0.6	0.3	1.7	1.6	0.9			
Subject 9 (After temperature conditioning)	0.3	0.5	0.2	1.5	0.1	0.5			
Subject 10 (After temperature conditioning)	0.4	1.5	1.7	1.5	0.3	1.1			

MNA LABORATUVARLARI SAN. TİC, LTD, ŞTİ.

MNA LABORATUVARLARI

TECHNICAL EVALUATION REPORT (65-20-02-R01)

TESTS	PARAMETER	PERFORMANCE LEVELS			RESULTS	PERFORMANCE LEVELS	EVALUATION
		FFP1	FFP2	FFP3			
Flammibility	Mask shall not burn burn for more than 5	ourn or not to continue to an 5 s		Flame not seen	-	PASS	
Carbondioxide content of the inhalation air	Shall not exceed an av	verage of % 1			0,55 0,53 0,50	-	PASS
Penetration of filter material	Sodium chloride, 95 L/min %, max	% 20	% 6	%1	See the table below	FFP2	PASS
	Paraffin oil, 95 L/min				See the table below	FFP2	PASS

Penetration of filter material	Sodium Chloride (%)	Paraffin Oil (%)	
As recieved	0.2	0.2	
As recieved	0.2	0.2	
As recieved	0.4	0.3	
After the simulated wearing treatment	0.3	0.2	
After the simulated wearing treatment	0.2	0.2	
After the simulated wearing treatment	0.4	0.2	
Mechanical strength and temperature conditioning	0.4	0.3	
Mechanical strength and temperature conditioning	0.2	0.3	
Mechanical strength and temperature conditioning	0.3	0.2	

TESTS	PARAMETER	PERFO LEVELS	RMANC S	Œ	RESULTS	PERFORMANCE LEVELS	EVALUATION
		FFP1	FFP2	FFP3			
Compatibility with skin	The same same same	e known to be likely to ny other adverse effect		Appropriate	-	PASS	
Head harness	It can be donned and	removed easily			Appropriate	-	PASS
Breathing Resistance	Inhalation 30L/min	0,6 mbar	0,7 mbar	1 mbar	See the table below	FFP2	PASS
	Inhalation 95L/min	2,1 mbar	2,4 mbar	3 mbar	See the table below	FFP2	PASS
	Exhalation 160L/min	50L/min 3 3 3 mbar mbar mbar			See the table below	FFP2	PASS

Breathing Resistance	Inhalation 30L/min	Inhalation 95L/min	
As recieved	0.3	1.4	
As recieved	0.3	1.4	
As recieved	0.2	1.3	
After temperature conditioning	0.2	1.3	



MNA LABORATUVARLARI

TECHNICAL EVALUATION REPORT (65-20-02-R01)

After temperature conditioning	0.3	1.4
After temperature conditioning	0.3	1.4
After the simulated wearing treatment	0.2	1.3
After the simulated wearing treatment	0.3	1.4
After the simulated wearing treatment	0.3	1.3

Breathing Resistance 160L/min	Facing directly ahead	Facing vertically upwards	Facing vertically downwards	Lying on the left side	Lying on the right side
As recieved	1,2	1,2	1,2	1,1	1,2
As recieved	1,1	1,2	1,2	1,1	1,1
As recieved	1,1	1,1	1,2	1,2	1,2
After temperature conditioning	1,2	1,2	1,2	1,1	1,2
After temperature conditioning	1,2	1,1	1,2	1,2	1,1
After temperature conditioning	1,1	1,1	1,1	1,2	1,2
After the simulated wearing treatment	1,1	1,2	1,2	1,2	1,2
After the simulated wearing treatment	1,2	1,2	1,2	1,2	1,1
After the simulated wearing treatment	1,1	1,2	1,2	1,2	1,1

9. DECISION PROPOSAL

Analysis and examinations LINDENCARE LP1 model coded personal protective equipment; Respiratory Protective Devices EN 149 + A1 - Filtered Half Masks for Protection Against Particles - Properties, Experiments and Marking standards are evaluated. It is recommended to be certified at the performance levels specified as a result of technical evaluations.

10. ATTACHMENTS

- Basic Health Safety Requirements
- Risk Assessment
- Test Reports
- User Instruction

Reason for revision: The material information has been revised.

CONTROLLER : VOLKAN AKIN

SING :

DATE : 17.11.2020